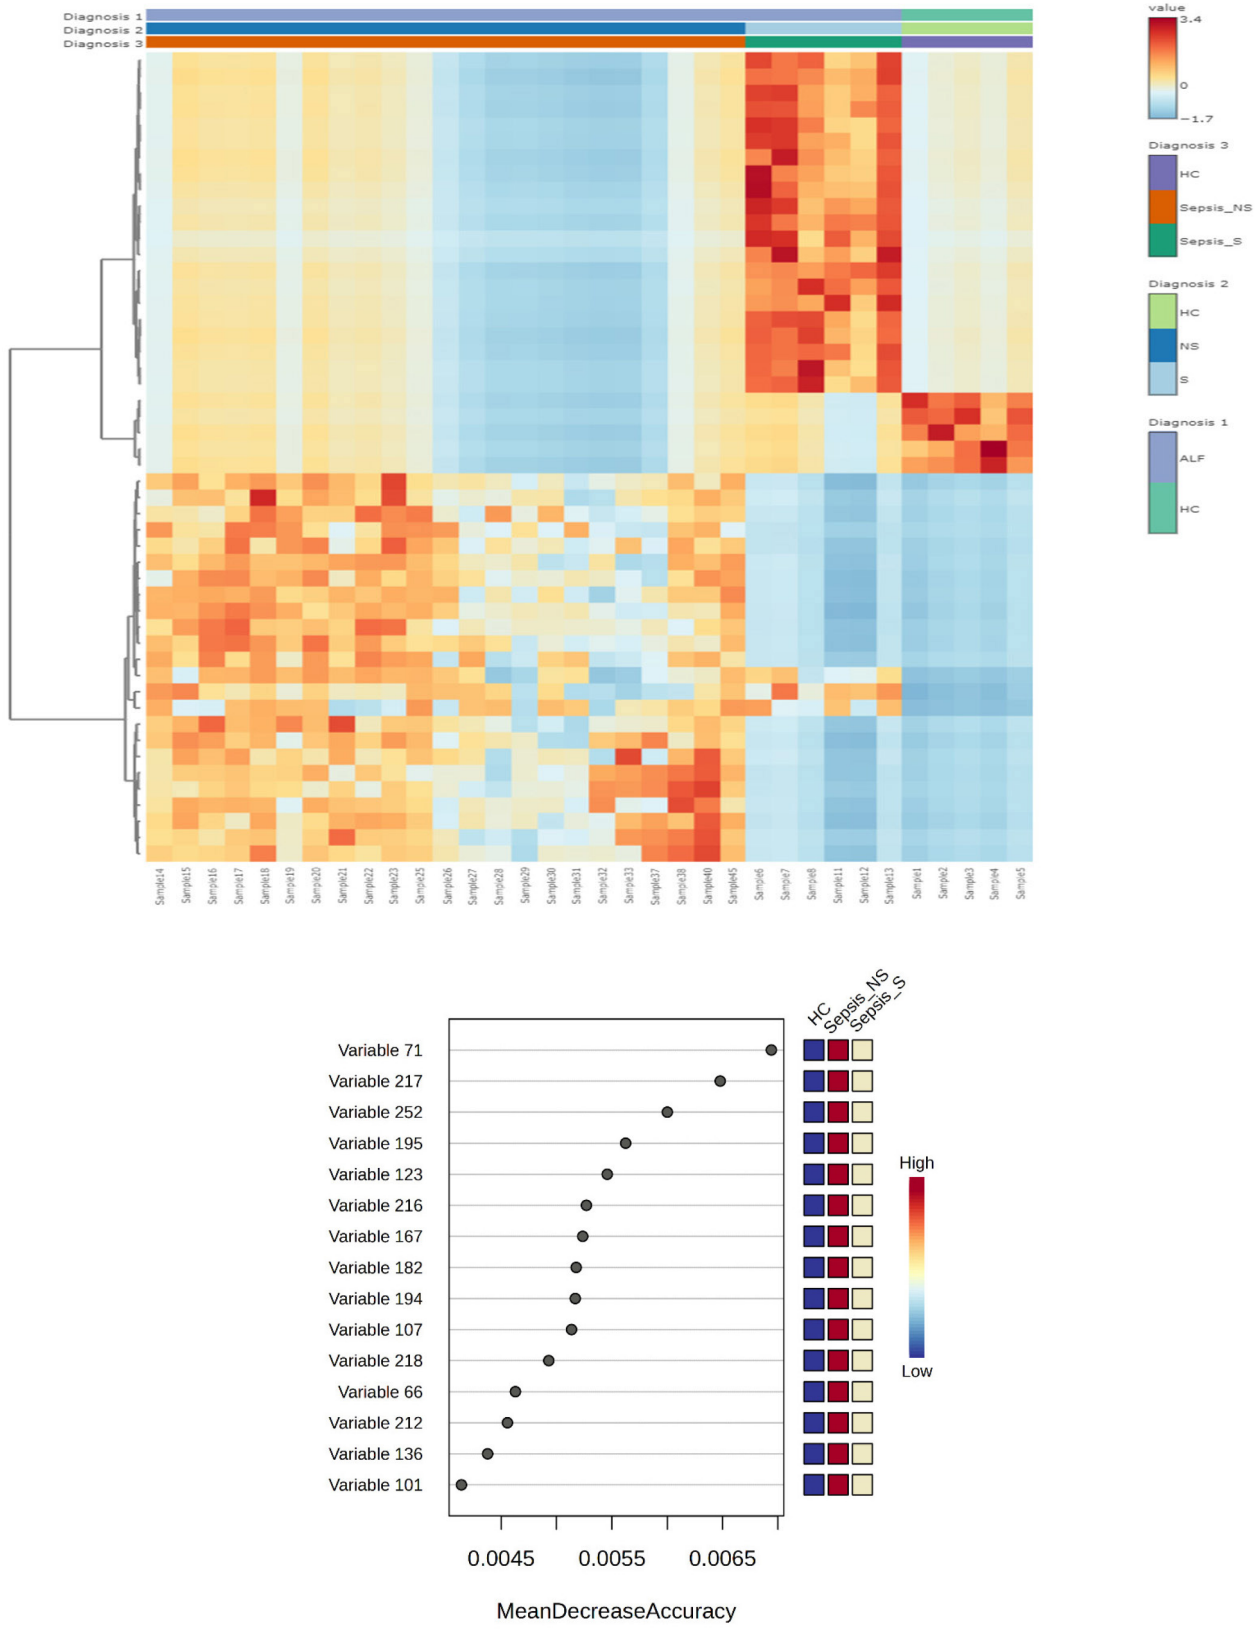

Supplementary Figure 16. Heatmap and mean decrease accuracy according to the sepsis as the etiology of the samples.